

FIG. 1

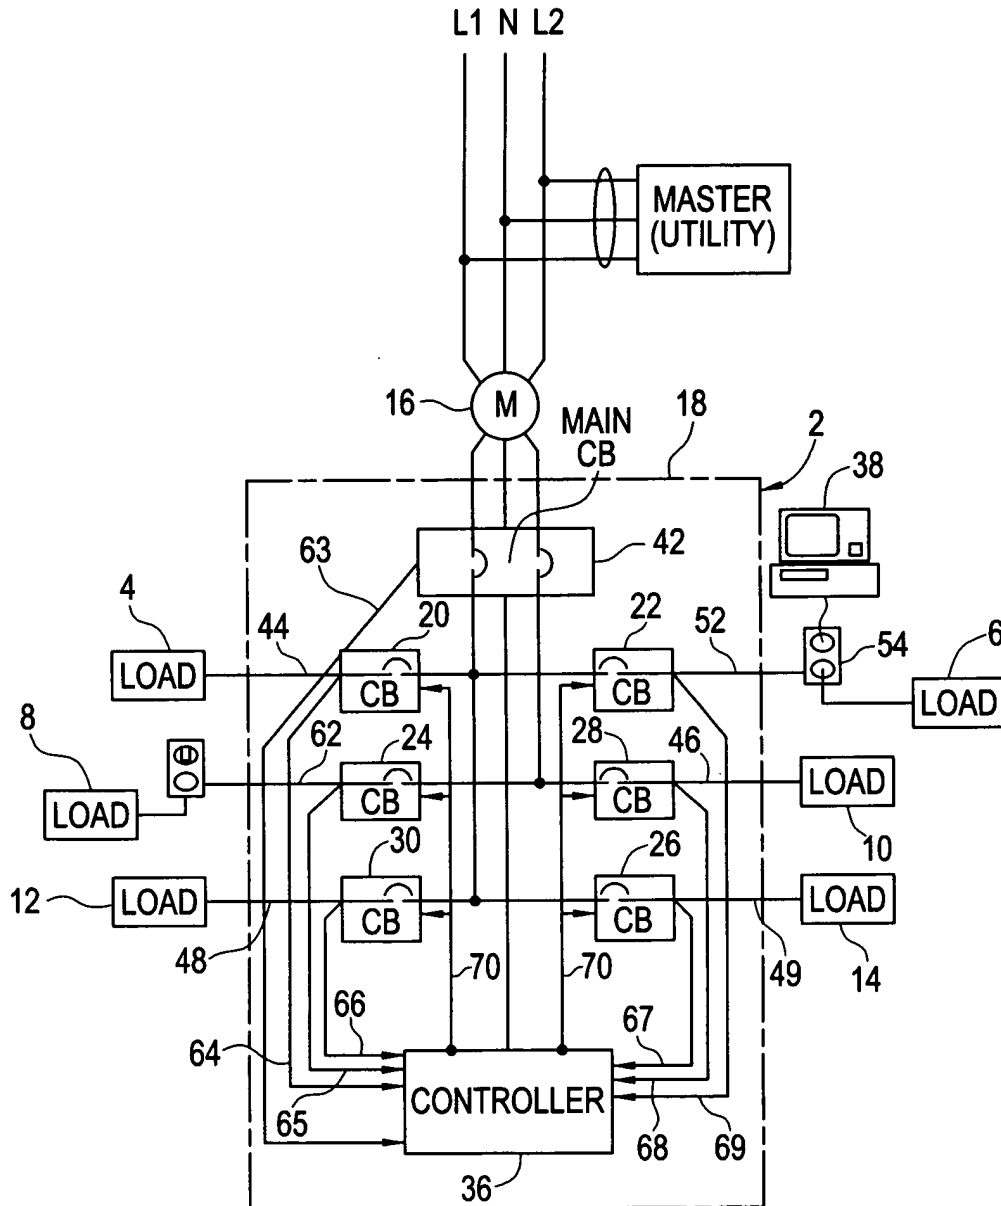


FIG. 2


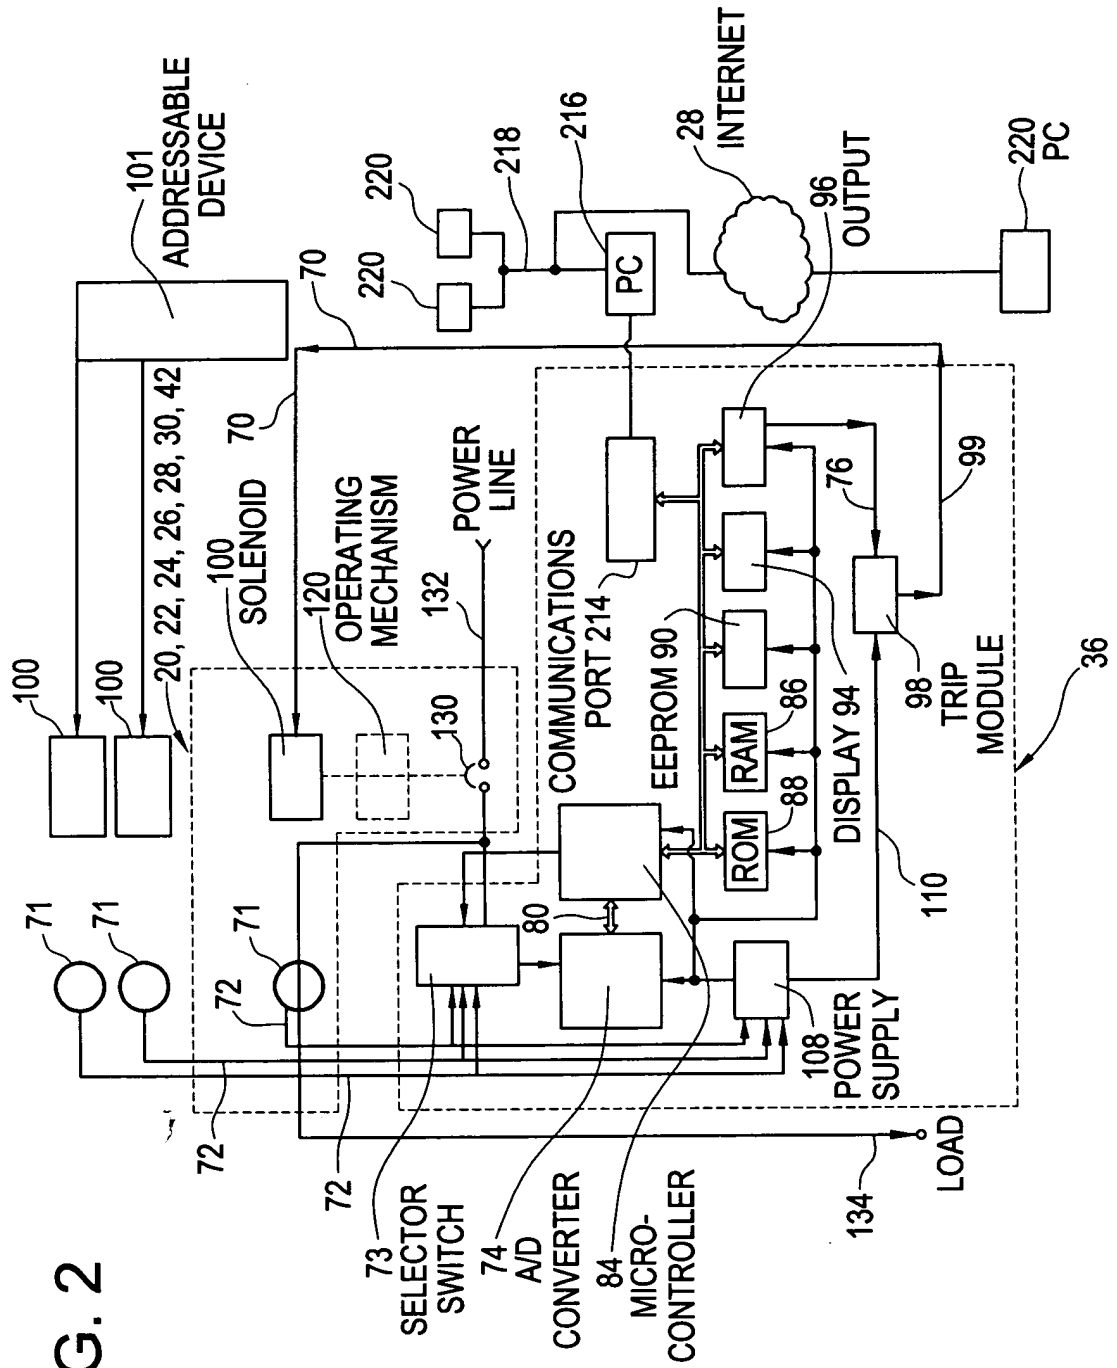


FIG. 3

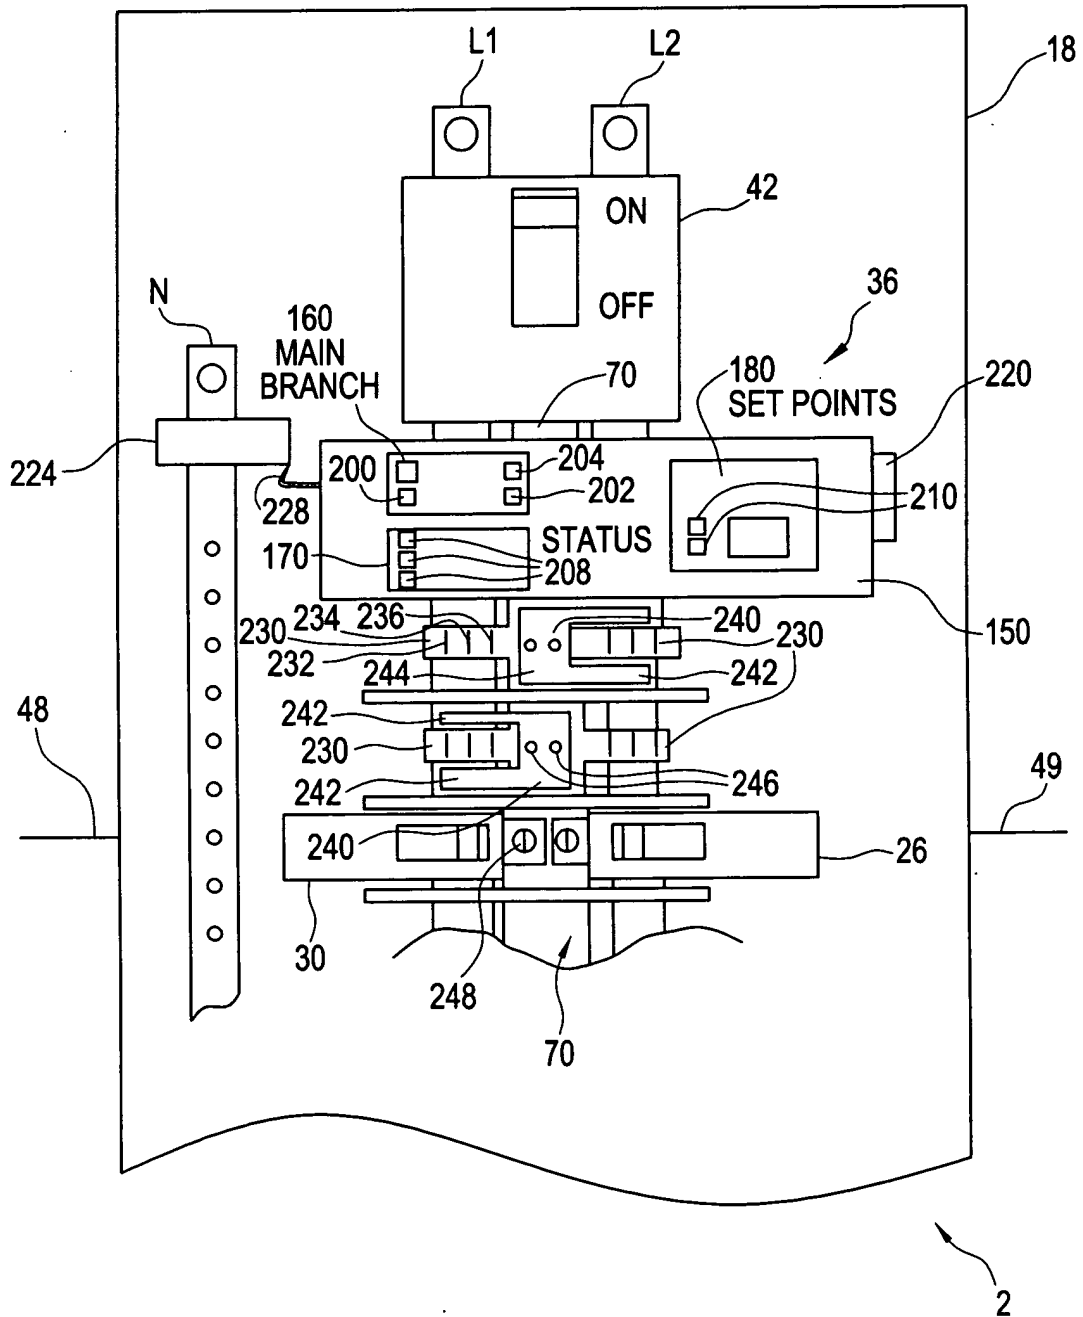

202120 96628960

FIG. 1 is a schematic diagram of a system 100 for processing a sample 134. The system 100 includes a housing 300 with a front panel 312 and a base 316. Inside the housing, a sample 134 is positioned on a stage 120. A probe 320 is used to interact with the sample. A control unit 36 is connected to the system via a cable 376. Various components are labeled with reference numerals: 100, 120, 134, 300, 312, 316, 320, 322, 324, 326, 332, 334, 338, 340, 342, 344, 346, 360, 362, 366, 370, 372, 374, 376.